TREND NETWORKS
High Wycombe, Buckinghamshire, United Kingdom
UK +44 (0)1925 428 380 DE +49 (0)89 99 686-0
US (973) 957-7700 FR +33 (0)1 69 35 54 70

Certificate of Calibration

This Certificate certifies that the items listed below have been tested, manufactured, calibrated and/or inspected in accordance with TREND NETWORKS procedures. These procedures are ISO 9001:2015 controlled and are designed to assure that the instrument will meet its published specification.

Inspections and/or tests and Calibration have been performed, as applicable at or on behalf of

TREND Networks
TREND Networks House
728 London Road, High Wycombe
Buckinghamshire. HP11 1HE. UK

Calibration compliance is achieved by comparison to calibrated standards, using an automated test process, in accordance with LanTEK IV Calibration Procedure 163646 on file at the above address. Procedure 163646 details the method of calibration showing traceability to reference artifacts with calibration certificates documenting traceability to the National Physical Laboratory (NPL) and or National Institute of Standards and Technology (NIST).

Certifier Information

Model: LanTEK IV-L 500

Calibration Date: 22 Sep 2026 Main S/N: 24250014

Calibration Due: 22 Oct 2027 Remote S/N: 24250003

Calibration Information

Test Standards: ANSI/TIA 1152-A Level 2G
ISO/IEC 61935-1 Ed.5 Level VI

Calibration Location: POLAND

Artifact Set Number: 04

Temperature: 23°C ±3°C

Recommended Calibration Period

12 Months for LanTEK IV cable certifiers.
A new tester may be shipped with a period of up to 15 months of valid calibration.
Testers returned for annual calibration will be shipped with a 12 month calibration period.

Summary


The tester is operational, all established measurement values are within specified manufacturing tolerances.


TREND NETWORKS
High Wycombe, Buckinghamshire, United Kingdom
UK +44 (0)1925 428 380
US (973) 957-7700
DE +49 (0)89 99 686-0
FR +33 (0)1 69 35 54 70


Calibration Certificate Test Data


Test Standards: ANSI/TIA 1152-A Level 2G
ISO/IEC 61935-1 Ed.5 Level VI


Model	Serial numbers: Main/Remote	Calibration Date
LanTEK IV-L 500	24250014 / 24250003	22 Sep 2026

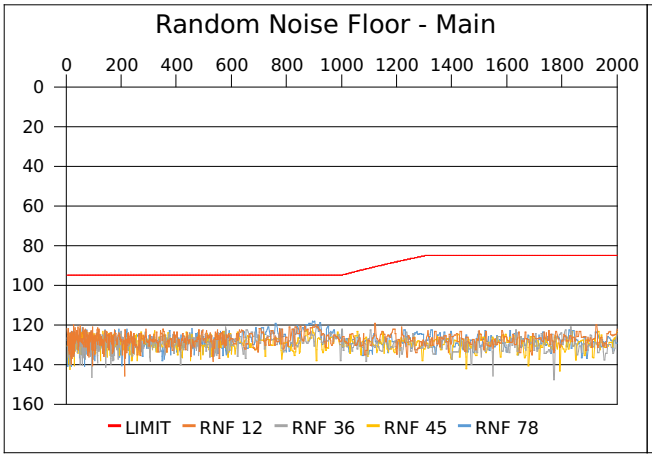


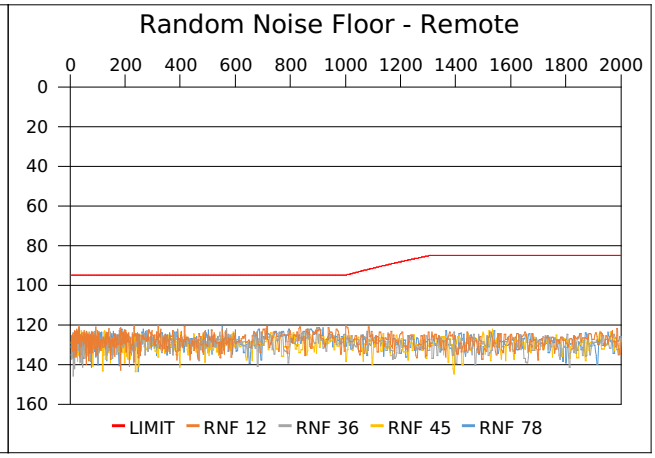

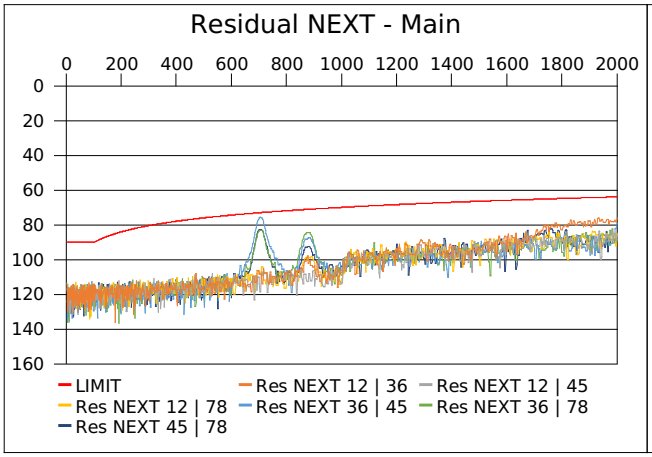


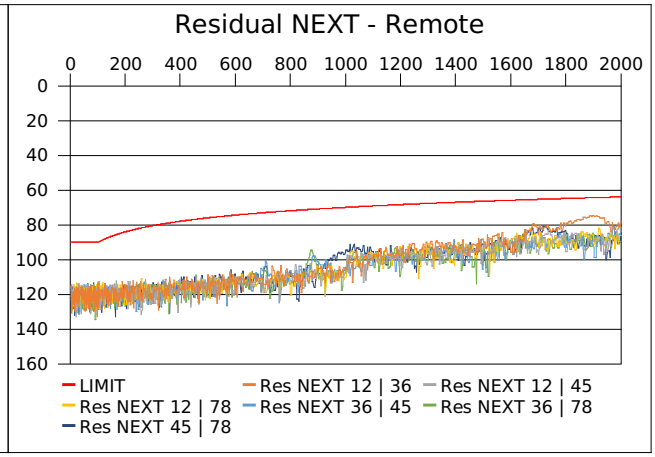


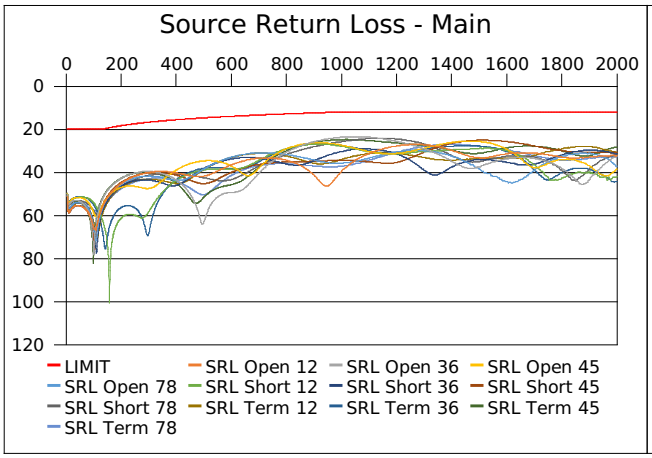


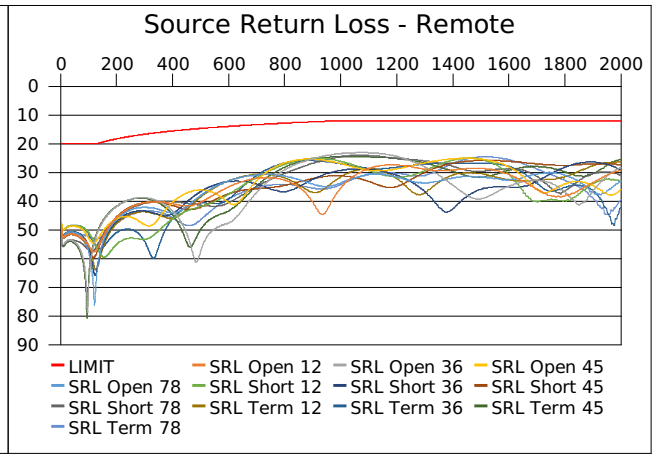



Model	Serial numbers: Main/Remote	Calibration Date
LanTEK IV-L 500	24250014 / 24250003	22 Sep 2026

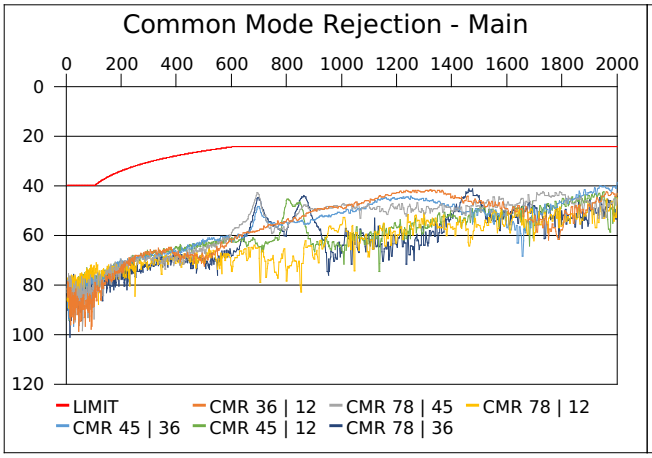


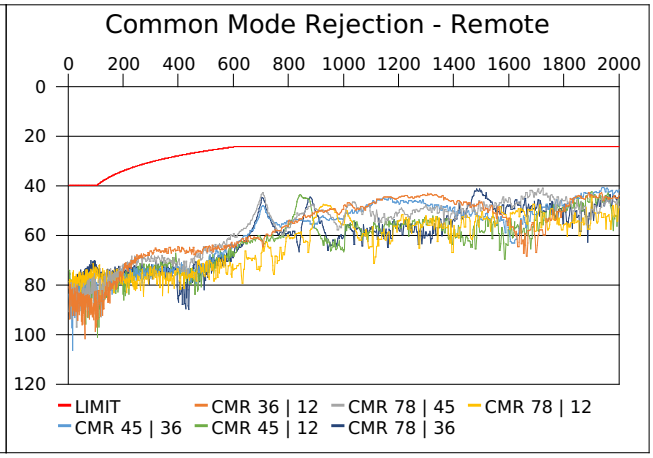

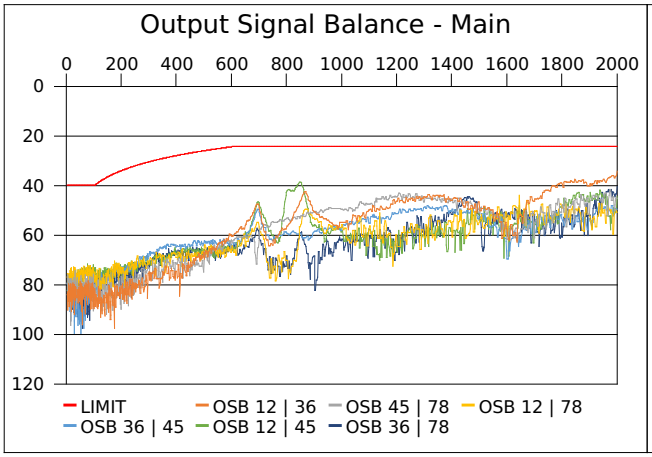

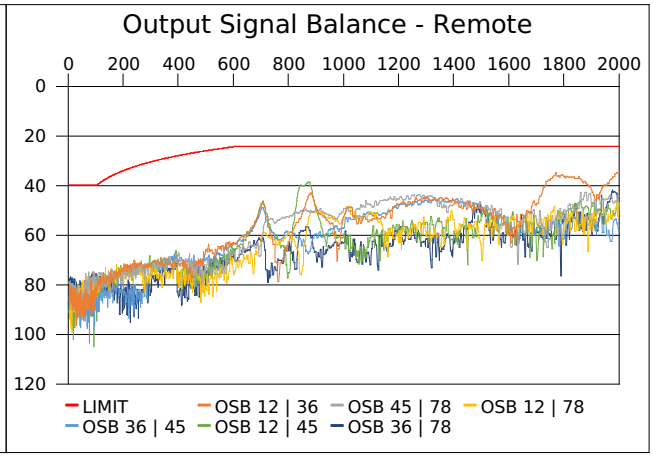

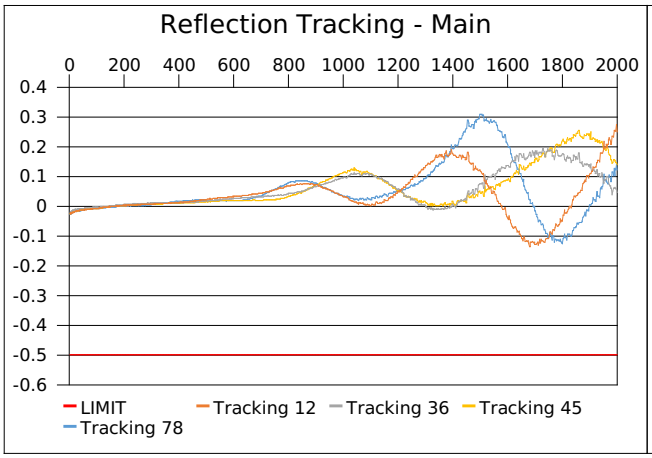

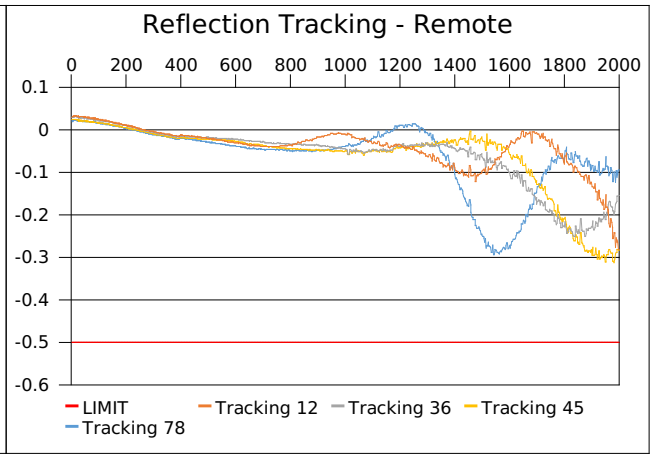

Model	Serial numbers: Main/Remote	Calibration Date
LanTEK IV-L 500	24250014 / 24250003	22 Sep 2026

