



Certificate of Calibration

This Certificate certifies that the items listed below have been tested, manufactured, calibrated and/or inspected in accordance with TREND NETWORKS procedures. These procedures are ISO 9001:2015 controlled and are designed to assure that the instrument will meet its published specification.

Inspections and/or tests and Calibration have been performed, as applicable at or on behalf of

TREND Networks
Stokenchurch House, Oxford Road
Stokenchurch, High Wycombe
Buckinghamshire. HP14 3SX. UK

Calibration compliance is achieved by comparison to calibrated standards, using an automated test process, in accordance with LanTEK IV Calibration Procedure 163646 on file at the above address. Procedure 163646 details the method of calibration showing traceability to reference artifacts with calibration certificates documenting traceability to the National Physical Laboratory (NPL) and or National Institute of Standards and Technology (NIST).

Certifier Information

Model: LanTEK IV 3000

Calibration Date: 28 Mar 2022

Main S/N: 19310040

Calibration Due: 28 Apr 2023

Remote S/N: 19310018

Calibration Information

Test Standards: ANSI/TIA 1152-A Level 2G
ISO/IEC 61935-1 Ed.5 Level VI

Calibration Location:
POLAND

Artifact Set Number: 07
Temperature: 23°C ±3°C

Recommended Calibration Period

12 Months for LanTEK IV cable certifiers.

A new tester may be shipped with a period of up to 15 months of valid calibration.

Testers returned for annual calibration will be shipped with a 12 month calibration period.




Summary

The tester is operational, all established measurement values are within specified manufacturing tolerances.

Calibration Certificate Test Data
Test Standards: ANSI/TIA 1152-A Level 2G
 ISO/IEC 61935-1 Ed.5 Level VI

 Model
 LanTEK IV 3000




 Serial numbers: Main/Remote
 19310040 / 19310018

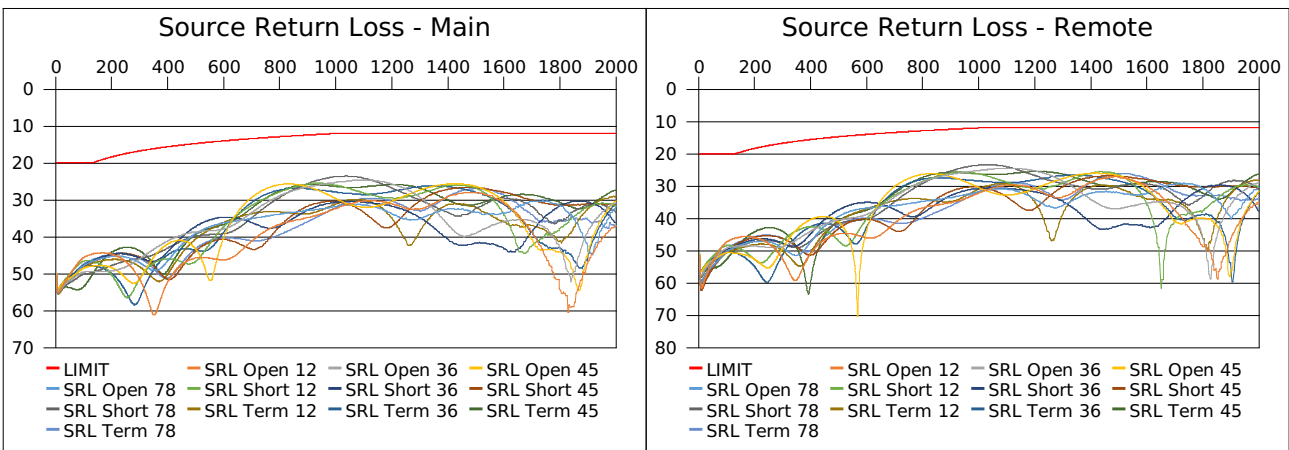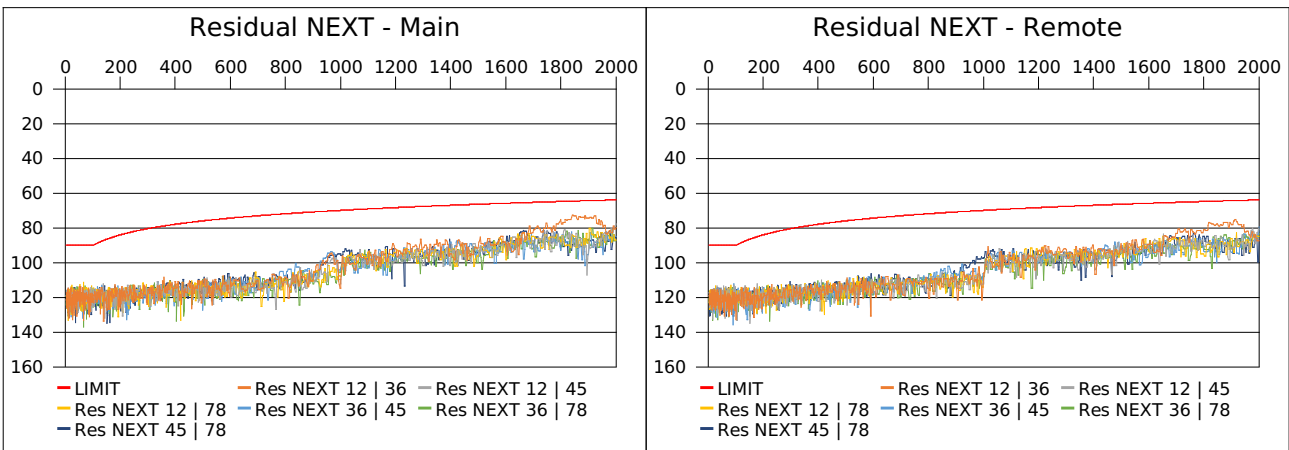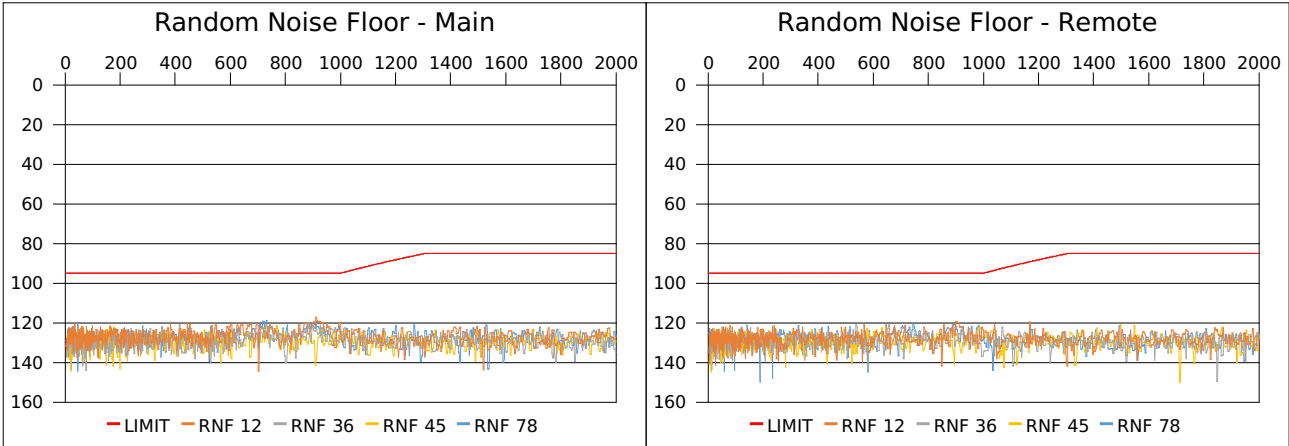 Calibration Date
 28 Mar 2022


Model
LanTEK IV 3000

Serial numbers: Main/Remote
19310040 / 19310018

Calibration Date
28 Mar 2022

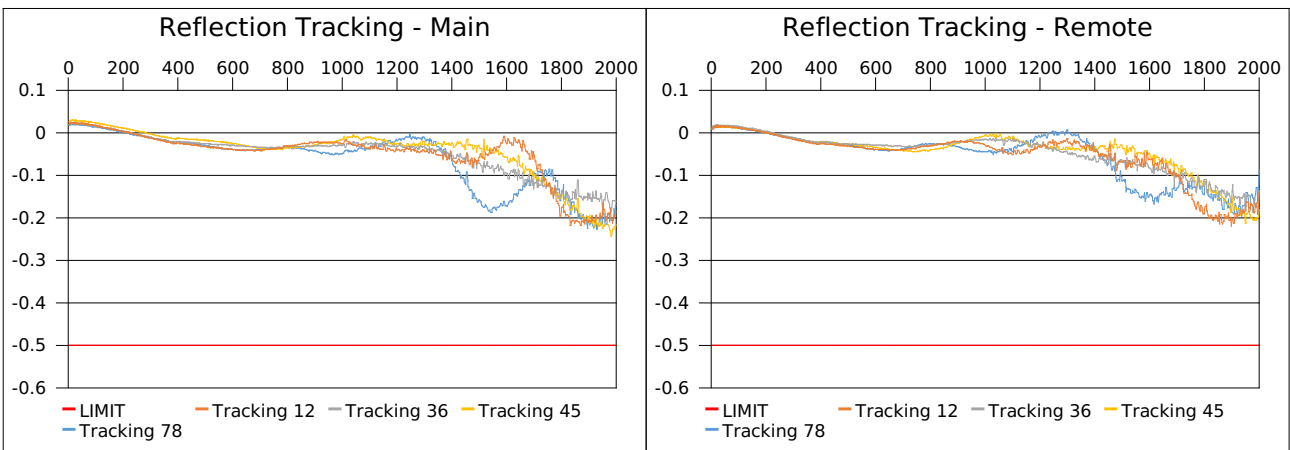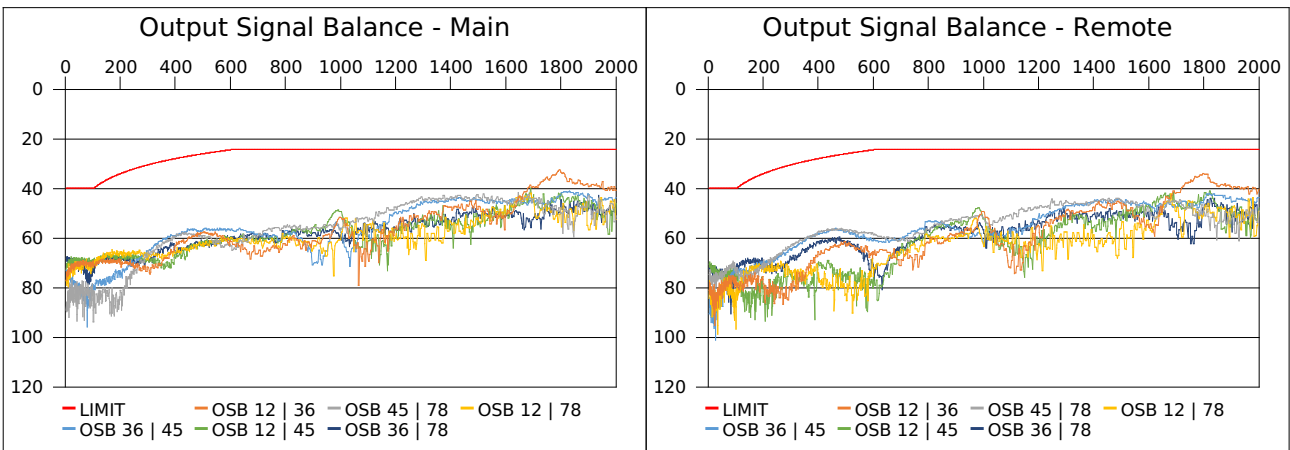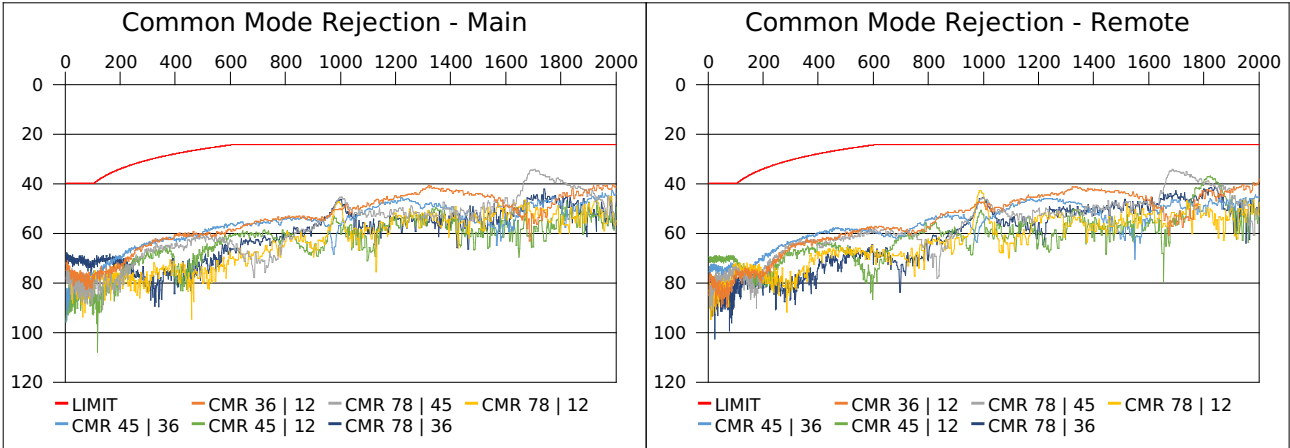



Model
LanTEK IV 3000

Serial numbers: Main/Remote
19310040 / 19310018

Calibration Date
28 Mar 2022

